

Report Documentation Page				Form Approved OMB No. 0704-0188	
Public reporting burden for the collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington VA 22202-4302. Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to a penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number.					
1. REPORT DATE 2005		2. REPORT TYPE		3. DATES COVERED 00-00-2005 to 00-00-2005	
4. TITLE AND SUBTITLE Valence Determination by Electron Energy Loss Spectroscopy of the Multi-Valence Metal Chromium				5a. CONTRACT NUMBER	
				5b. GRANT NUMBER	
				5c. PROGRAM ELEMENT NUMBER	
6. AUTHOR(S)				5d. PROJECT NUMBER	
				5e. TASK NUMBER	
				5f. WORK UNIT NUMBER	
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) Naval Research Laboratory, Oceanography Division, Stennis Space Center, MS, 39529				8. PERFORMING ORGANIZATION REPORT NUMBER	
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES)				10. SPONSOR/MONITOR'S ACRONYM(S)	
				11. SPONSOR/MONITOR'S REPORT NUMBER(S)	
12. DISTRIBUTION/AVAILABILITY STATEMENT Approved for public release; distribution unlimited					
13. SUPPLEMENTARY NOTES Microscopy and Microanalysis 2005, July 31 - Aug. 4, 2005, Honolulu, Hawaii					
14. ABSTRACT					
15. SUBJECT TERMS					
16. SECURITY CLASSIFICATION OF:			17. LIMITATION OF ABSTRACT Same as Report (SAR)	18. NUMBER OF PAGES 2	19a. NAME OF RESPONSIBLE PERSON
a. REPORT unclassified	b. ABSTRACT unclassified	c. THIS PAGE unclassified			

Valence Determination by Electron Energy Loss Spectroscopy of the Multi-Valence Metal Chromium

T. L. Daulton* and B. J. Little**

*Marine Geosciences Division, **Oceanography Division
Naval Research Laboratory, Stennis Space Center, MS 39529, USA

Chromium is a redox active 3d transition metal with a wide range of valences (-2 to +6) that control the geochemistry and toxicity of the element. A variety of Cr-bearing minerals [1] are found in meteorites of all petrographic classes [2], lunar basalts [3], Martian rocks, and the Earth, recording valuable information concerning geochemical conditions of mineralization. Natural weathering of Cr-bearing minerals [4] and fallout of volcanic ash release Cr into the terrestrial environment. Furthermore, Cr compounds are widely used in numerous industrial processes [5] which can discharge toxic Cr complexes in soils/sediments and surface/ground waters, as well as the atmosphere in the form of aerosols. Therefore, techniques that measure Cr valence are important bio/geochemical tools. Until now, all established methods to determine Cr valence were bulk techniques with many specific to a single, or at best, only a few oxidation state(s). We report electron energy loss spectroscopy (EELS) techniques that, unlike other methods, can determine Cr valence at high-spatial resolution (nm-scale) over a wide valence range, Cr(0) to Cr(VI).

In this work, the fine structure of Cr-L_{2,3} edges was parametrized by measurement of the chemical shift of the L₃ edge and the ratio of integrated intensity under the L₃ and L₂ edges (Table 1). These parameterizations were correlated to Cr valence for a large suite of standards (Fig. 1). Valence of an unknown can be determined by comparing its fine structure parameterizations to that of the standards. Measurement of the L₃/L₂ ratio is highly dependent on the post-edge background subtraction. The background was modeled by a fit to a 2 eV wide window positioned 4.8 eV above the L₂ maximum. The fit was extrapolated to the L₂ maximum where a step was inserted and then was extrapolated to the L₃ maximum. A second step function was inserted at the L₃ maximum and set to zero below the maximum (Fig. 2). The ratio for the step heights was initially set as 2, but was refined by iteration by assigning the step height the value of the L₃/L₂ ratio determined after each iteration. Intensity of the L edges was measured by integrating a 5 eV wide region centered with respect to the edge maxima.

Our results demonstrate that other factors in addition to valence, e.g. crystal field splitting (i.e, atom coordination, low- or high-spin configuration), spin-orbit interactions, atomic coulomb repulsion, and exchange effects, can significantly influence the fine structure of Cr-L_{2,3} adsorption edges. Consequently, measurement of the L₃ peak position and the ratio of L₃/L₂ integrated peak intensity must be used together to unambiguously determine Cr valence if the full range of oxidation states is considered. However, even with two parameterizations it is difficult to distinguish Cr(IV) and low-spin Cr(II) compounds from Cr(III). Nevertheless, when Cr is known divalent, low- and high-spin *dⁿ* orbital configurations can be readily distinguished.

References:

- [1] V. M. Burns & R. G. Burns, *Geochim. Cosmochim. Acta* **39**, 903-910 (1975).
- [2] T. E. Bunch & E. Olsen, *Geochim. Cosmochim. Acta* **39**, 911-927 (1975).
- [3] S. R. Sutton *et al.*, *Geochim. Cosmochim. Acta* **57**, 461-468 (1993).
- [4] J. Robles-Camacho & M. Armienta, *J. Geochem. Explor.* **68**, 167-181 (2000).
- [5] M. E. Losi *et al.*, *Rev. of Environ. Contam. & Toxicol.* **136**, 91-121 (1994).

Table 1.
Fine Structure Parameterizations

Standard	L ₃ Peak (eV)	L ₃ /L ₂
Cr(0)		
Cr ₂₃ C ₆	578.03 (5)	1.498 (3)
Cr(CO) ₆	579.06 (7)	1.520 (7)
Cr	577.18 (2)	1.525 (3)
Cr(I)		
(C ₆ H ₆) ₂ CrI	576.87 (3)	1.798 (6)
Cr(II)		
[(CH ₃) ₄ C ₅ H] ₂ Cr	578.43 (4)	1.715 (4)
Cr ₂ (CH ₃ COO) ₄ •2(H ₂ O)	578.55 (3)	1.720 (2)
[(CH ₃) ₅ C ₅] ₂ Cr	578.35 (2)	1.757 (3)
CrSe	576.65 (5)	2.004 (13)
CrCl ₂	577.11 (4)	2.184 (17)
CrF ₂	576.78 (3)	2.246 (14)
Cr(III)		
CrPO ₄ •4H ₂ O	579.74 (6)	1.546 (3)
KCr(SO ₄) ₂ •12H ₂ O	579.77 (4)	1.559 (5)
CrCl ₃	578.13 (2)	1.638 (3)
(Fe,Mg)(Cr,Al,Fe) ₂ O ₄	578.89 (2)	1.646 (2)
NdCrO ₃	579.35 (3)	1.675 (7)
LaCrO ₃	578.71 (2)	1.704 (4)
Cr ₃ (CH ₃ COO) ₇ (OH) ₂	578.47 (2)	1.709 (2)
Cr ₂ O ₃	578.81 (3)	1.712 (5)
Cr(IV)		
CrO ₂	579.70 (3)	1.548 (2)
Cr(V)		
NdCrO ₄	580.43 (3)	1.414 (4)
Cr(VI)		
PbCrO ₄	581.85 (7)	1.370 (5)
K ₂ Cr ₂ O ₇	582.83 (3)	1.408 (6)
K ₂ CrO ₄	581.77 (2)	1.474 (4)
Na ₂ CrO ₄	582.26 (3)	1.475 (6)

Spectrometer calibrated to yield 855.0 eV for Ni-L₃ edge maximum of NiO. Standard error of mean (for upwards of 30 measurements) is given by (n), e.g. for Cr₂₃C₆: 1.498 (3) = 1.498 ± 0.003.

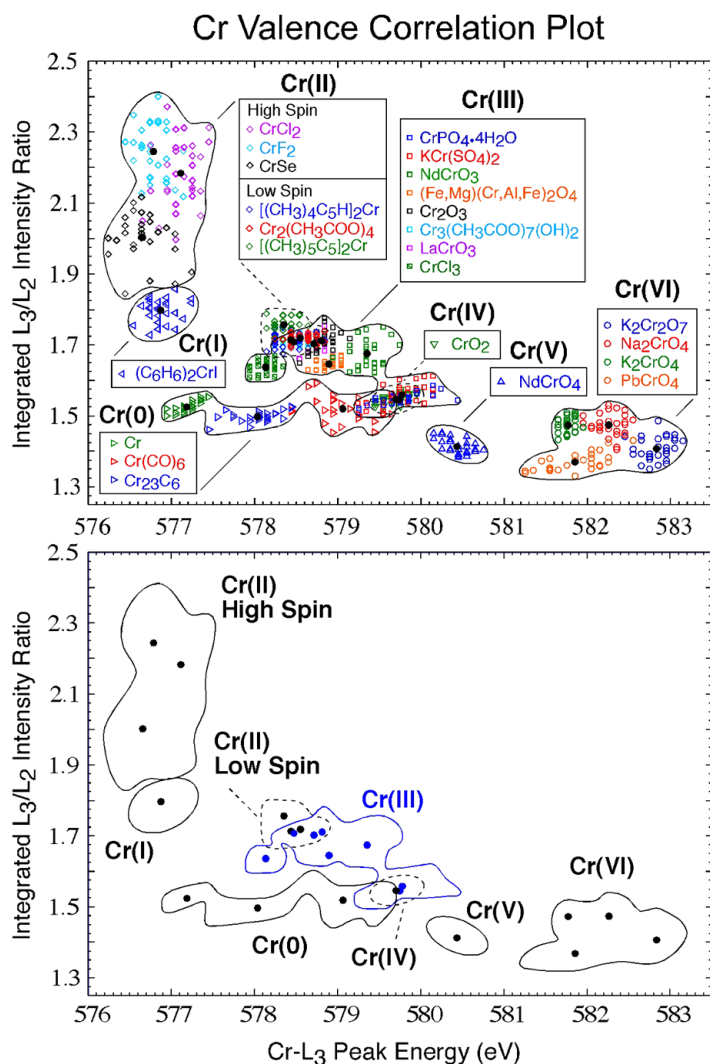


Figure 1. The correlation between measured L₃/L₂ integrated-peak intensity ratios and L₃ peak positions for Cr oxidation-state standards. The black, solid circles represent the mean of the data for a particular Cr standard. The regions bounded by closed curves are visual guides.

Figure 2. Post-edge background subtraction method used to measure the L₃/L₂ ratio. The bold line is the modeled background determined by a fit to a 2 eV wide window that starts 4.8 eV above the L₂ maxima.

